

Systematic Review

Comparative Evaluation of the Accuracy of Electronic Apex Locator and Digital Radiography for Working Length Determination in Primary Teeth: A Systematic Review

Ishita Agrawal¹, BDS; Farhin Katge², MDS; Sanmati Pol³, MDS; Devendra Patil³, MDS; Vamsi Krishna Chimata⁴, MDS; Debapriya Pradhan², MDS;

¹ Postgraduate Student, Dept. of Pediatric and Preventive Dentistry, Terna Dental College, Sector-22, Nerul West, Navi-Mumbai, India.

² Dept. of Pediatric and Preventive Dentistry, Terna Dental College, Sector-22, Nerul West, Navi-Mumbai, Maharashtra, India.

³ Lecturer, Dept. of Pediatric and Preventive Dentistry, Terna Dental College, Sector-22, Nerul West, Navi-Mumbai, Maharashtra, India.

⁴ Reader, Dept. of Pediatric and Preventive Dentistry, Terna Dental College, Sector-22, Nerul West, Navi-Mumbai, Maharashtra, India.

KEY WORDS

Dental Radiovisiography;
Digital Dental Radiography;
Primary Dentitions;
Milk Tooth;

Received: 28 December 2022;

Revised: 1 May 2023;

Accepted: 22 July 2023;

Copyright

© Journal of Dentistry, this is an open access article distributed under the terms of the Creative Commons Attribution 4.0 International License, (<http://creativecommons.org/licenses/by/4.0/>) which permits reusers to copy and redistribute the material in any medium or format if the original work is properly cited, and attribution is given to the creator. The license also permits for commercial use.

ABSTRACT

Statement of the Problem: It is challenging to perform a pulpectomy procedure in primary tooth because of its physiological root resorption and variation in root morphology. Working length measurement is considered to be one of the critical steps, as it determines the extent of obturation and apical seal.

Purpose: To compare the accuracy of electronic apex locator (EAL) and digital radiography (DR) for working length determination in primary teeth.

Materials and Method: In this systematic review, electronic databases and grey literature were searched from 1st January 2005 to 1st January 2023 for randomized control trial, non-randomized control trial, *in vitro* studies, *ex vivo* studies that compared accuracy of EAL and DR in primary teeth. Two reviewers independently identified studies, retrieved data, and assessed risk of bias using the revised and validated MINORS (methodological index for non-randomized studies) criteria.

Results: Ten studies were included in qualitative analysis. Seven out of ten studies showed low risk of bias whereas other three studies showed high risk of bias. In view of methodological heterogeneity of the findings, a meta-analysis was not conducted.

Conclusion: Available evidence suggests a moderate quality of evidence in this systematic review. Analyzing the ten studies included in this systematic review, the majority of studies showed statistically insignificant difference between EAL and DR. However, EAL was closer to actual WL as compared to DR. Based on the evidence that is currently available; EAL can be considered as an alternative for working length measurement in primary teeth.

Corresponding Author: Katge F, Dept. of Pediatric and Preventive Dentistry, Terna Dental College, Sector-22, Nerul West, Navi-Mumbai, Maharashtra, India. Email: pedotdc@gmail.com

Cite this article as: Agrawal I, Katge F, Pol S, Patil D, Krishna Chimata V, Pradhan D. Comparative Evaluation of the Accuracy of Electronic Apex Locator and Digital Radiography for Working Length Determination in Primary Teeth: A Systematic Review. *J Dent Shiraz Univ Med Sci.* September 2024; 25(3): 203-214.

Introduction

Pediatric endodontic procedure helps in maintaining teeth in dentition, until their normal exfoliation time [1]. An accurate evaluation of root canal length determines the success of an endodontic procedure.

American Academy of Endodontics (2003) defined working length as 'the distance from a coronal reference point to the point at which canal preparation and filling should terminate' [2]. Accurate working length (WL)

determination is extremely important, as it has an impact on ideal canal preparation, disinfection, and apical seal of root canal system [3]. The correct root canal length of primary teeth is difficult to predict because of the root resorption pattern, which could be either physiological or pathological. There is continuous alteration in size, shape, and position of root apices of primary teeth, [4] that causes difficulty in accurate determination of root canal length [5]. Traditional methods for estab-

lishing WL include conventional radiography, tactile sensation, moisture on a paper point, and knowledge of root canal anatomy.

After the introduction of digital radiography (DR), the first commercial integrated digital imaging system in dentistry was radiovisiography (RVG) which comprises an intraoral sensor instead of the conventional X-ray film [6]. DR is based on digital image capture and uses a charge-coupled device [3]. The advantages of a digital radiography above the conventional method are; predominantly a faster image procurement, lower radiation dose and image editing ability [7]. Although both conventional and DR methods offer some advantages, such as direct observation of root canal anatomy, presence of any periapical lesion and canal curvatures, there are limitations associated with them, such as radiation exposure and image distortion, which results in difficulty in identification of resorbed root apices [3]. Electronic apex locators (EAL) have been introduced to overcome the disadvantages of the above techniques. It is used in dentistry to determine where the apical constriction is located in the root canal [8]. It is a more accurate, easy, and painless technique, which is very useful in uncooperative children. Various advantages of EAL include; lesser radiation dosage as well as procedure time, which helps in maintaining patient cooperation. The efficacy of EAL has been proven even in the presence of root resorption, which is frequently encountered in primary teeth [9]. Considering the importance of WL determination for pediatric endodontic treatment and its maintenance until normal exfoliation, the aim of this systematic review was to compare the accuracy of EAL and DR for WL determination in primary teeth.

Materials and Method

Protocol registration and review reporting

The present systematic review was registered with protocol ID CRD42020222326 at the International Prospective Register of Systematic Reviews (PROSPERO). This systematic review was reported according to Preferred Reporting Items for Systematic Reviews and Meta-Analyses checklist (PRISMA 2020) [10].

Research question

Research question for this systematic review was structured in PICOS format (participant, intervention, comparison, outcome and study design), depicted in Table 1.

Table 1: Population Intervention Comparison Outcome Study design (PICOS); EAL: Electronic apex locator, RVG: Radiovisiography, WL: Working length

Population	Human Primary Teeth
Intervention	EAL
Comparison	Radiovisiography (RVG)
Outcome	Working length (WL)
Study design	Randomized control trial, non-randomized control trial, <i>in vitro</i> studies, <i>ex vivo</i> studies.

Is there a difference in accuracy between an EAL and DR for WL determination in primary teeth?

Eligibility criteria

The eligibility criteria (Table 2) in this study were formulated to find studies based on the PICOS format. All studies were chosen in accordance with the criteria specified in this review.

Information sources and search strategy

Databases used in the search strategy included; Cochrane Library, National Library of Medicine (MEDLINE PubMed), Google scholar, EBSCOhost, Open grey literature, including both electronic and printed literature. The concept table (Table 3) denotes the terms used for search strategy, which included key concepts, as well as free text terms. Boolean operators such as OR/AND were used to combine search terms with other keywords relating to the review's goal. Additional articles were searched by looking through the references of the chosen publications, as well as previously published reviews on the topic, textbooks and publications, that met the inclusion criteria of the study.

Table 2: Eligibility criteria for qualitative assessment of studies (based on PICOS)

Inclusion Criteria	Exclusion Criteria
<ul style="list-style-type: none"> • Randomized control trial, non-randomized control trial, <i>in vitro</i> studies, <i>ex vivo</i> studies • Studies performed on primary teeth • Studies comparing electronic apex (EAL) and radiovisiography (RVG) to evaluate working length • Well defined information on working length using EAL and radiovisiography (RVG) • Articles published until 31st August 2021 • Articles published in English or which can be translated into english 	<ul style="list-style-type: none"> • Case reports, case series, reviews, book chapters, expert opinion, animal studies • Articles reporting medically compromised patients • Only abstracts

Table 3: Concept table

	Population	Intervention	Comparison	Outcome
Key concept	Human primary teeth	Electronic apex locator	Radiovisio-graphy	Working length determination
Free terms / Text words / TIAB terms	Deciduous dentition Deciduous teeth Deciduous molar Primary teeth Baby teeth Milk teeth Primary dentition Primary molars	Apex locators Formatron D10 Root Zx DentaPort ZX Propex II Root Zx Mini COXO C Smart-1 PRO iPex Apex ID	Digital radiography Digital radiovisio-graphy Radiography Dental digital radiography Digital dental radiography	Working length Working length measurement Apex localization Root length determination Root canal length
MeSH terms	Tooth Deciduous		Radiography Dental Digital	

Articles published or studies conducted from January 1, 2005 to January 31, 2023 were included for this systematic review.

Study selection

Selection of a study was done in three stages. In stage one, assessment of all the titles of the studies obtained through search strategy were done by two independent reviewers (IA and SP). Stage 2 involved screening of the abstracts, which was followed by screening of the full texts of relevant studies in stage 3. In case of disagreements between the two reviewers, a third reviewer (FK) was called in for a final decision. Only studies with full text reports were examined in this systematic review. Due to differences in the data supplied in abstract and those provided in the final report [11], literature published only as abstracts were excluded from the study. Authors were contacted for a full text of the relevant abstracts wherever possible.

Data collection and data items extracted

After defining the inclusion criteria for the selected articles, data extraction was performed independently by two review authors (IA and SP). Any disagreements in data extraction from the selected studies were discussed and resolved by a third (FK) and fourth (DP) reviewer. This information included authors name, year of publication, number of teeth included, demographic details of the patients (age in years), intervention, comparison, outcomes, study design and results.

Study of risk of bias assessment

The risk of bias assessment was performed by two independent reviewers (IA & SP); using a modified version of the methodological items for nonrandomized studies (MINORS) scale (Annexure 1) [12]. A third reviewer (FK) validated all modifications to the MINORS scale.

Cohen kappa coefficient for overall inter reviewer reliability was 0.725, indicating moderate agreement [13]. Any disagreements regarding risk of bias assessment, between the two reviewers (IA & SP), were resolved by a consensus between third (FK) and fourth (DP) reviewer. The items in MINORS scale were scored 0 (if not reported), 1 (if reported but inadequate) or 2 (if reported but adequate). The ideal score for comparative studies is 24. The checkpoints 6, 7 and 10 were excluded, as it was not applicable for this review. Hence, for the present systematic review 9 check-points were considered. The total score considered for the present review was 18. The score reported between 1 and 11 indicated high risk of bias, whereas score between 12 and 18 indicated low risk of bias.

Outcomes and data synthesis

The mean differences and their standard deviations were extracted and used in the presentation of results. The meta-analysis was not performed due to a high degree of heterogeneity seen in data extraction from different studies and methodologies.

Results

Study selection

PRISMA flowchart (2020) describing the process of selecting studies is shown in Figure 1 (Page et al. 2020). Electronic literature search yielded 746 results. In the initial step of the screening process, duplicates were removed (299) using Mendeley software for Windows (Mendeley Ltd, Version 1803 Elsevier, London UK). A total of 447 articles were then evaluated, in accordance to the PRISMA standards [10]. In the next step of the screening process, 409 articles were removed due to irrelevance based on titles and abstracts. Finally, 38 full text

Table 4: The excluded studies are as follows: (EAL: Electronic apex locator, WL: Working length, SD: Standard deviation, CBCT: Cone beam computed tomography, DR: Digital radiography)

Sr. no	Author and Year	Title	Reason for exclusion
1.	Shanmugaraj M, et al. (2007) [14]	Evaluation of working length determination methods: an <i>in vivo</i> / <i>ex vivo</i> study	They have included permanent teeth with mature apices
2.	Krajczár K, et al. (2008) [15]	Comparison of radiographic and electronic working length determination on palatal and mesio-buccal root canals of extracted upper molars	They have included permanent molar teeth. They haven't specified gold standard method
3.	Krajczár K, et al. (2008) [16]	Direct comparison of working length determination by ProPex electronic apex locator and radiographic method--an <i>in vitro</i> study	They have included permanent molar teeth. They haven't specified gold standard method
4.	Ravanshad S, et al. (2010) [17]	Effect of working length measurement by electronic apex locator or radiography on the adequacy of final working length: A randomized clinical trial	they have included 20 to 65 years age group patient who presented for endodontic therapy
5.	Cianconi L, et al. (2010) [18]	Accuracy of three electronic apex locators compared with digital radiography: an <i>ex vivo</i> study	They selected periodontally involved human teeth extracted from 35- to 60-year-old patients
6.	Real DG, et al. (2011) [19]	Accuracy of working length determination using 3 electronic apex locators and direct digital radiography	Twenty extracted human maxillary premolars were selected
7.	Parekh V, et al. (2011) [20]	Comparative study of periapical radiographic techniques with apex locator for endodontic working length estimation: an <i>ex vivo</i> study	They have included premolar teeth
8.	Vieyra JP, et al. (2010) [21]	Comparison of working length determination with radiographs and two electronic apex locators	They have included permanent teeth
9.	Vieyra JP, et al. (2011) [22]	Comparison of working length determination with radiographs and four electronic apex locators	They have included permanent teeth
10.	Saritha S, et al. (2012) [23]	Clinical evaluation of Root ZX II electronic apex locator in primary teeth	They haven't taken any gold standard method for comparison
11.	Singh SV, et al. (2012) [24]	An <i>in vivo</i> comparative evaluation to determine the accuracy of working length between radiographic and electronic apex locators	They included 20 patient aged 25 to 55 years undergoing extraction because of periodontal and orthodontic reasons
12.	Kishor KM (2012) [25]	Comparison of working length determination using apex locator, conventional radiography and radiovisiography: an <i>in vitro</i> study	They have included permanent maxillary central incisors
13.	Mandlik J, et al. (2013) [26]	An <i>in vivo</i> evaluation of different methods of working length determination	They have included premolar and supernumerary teeth
14.	Oznurhan F, et al. (2014) [27]	Clinical evaluation of apex locator and radiography in primary teeth	They haven't taken any gold standard method for comparison
15.	Basso MD, Jeremias F, Cordeiro RC, Santos-Pinto L (2015) [28]	Digital radiography for determination of primary tooth length: <i>in vivo</i> and <i>ex vivo</i> studies	They compared accuracy of radiographic tooth length obtained from <i>in vivo</i> digital radiograph with that obtained from <i>ex vivo</i> digital radiograph
16.	Singh D, et al. (2015) [29]	Comparative evaluation of adequacy of final working length after using Raypex5 or radiography: an <i>in vivo</i> study	They included patient aged 20 to 45 years who presented for endodontic therapy
17.	Carneiro JA, et al. (2016) [30]	Comparison of working length determination using apex locator and manual method <i>ex vivo</i> study	They have included permanent single rooted teeth. They compared electronic measurement with manual method
18.	Dutta K, et al. (2017) [31]	Comparative evaluation of three methods to measure working length - Manual tactile sensation, digital radiograph, and multi detector computed tomography: An <i>in vitro</i> study	They compared working length with three different methods manual tactile sensation, digital radiograph and Multi detector computed tomography.
19.	Khateeb SU, et al. (2017) [32]	Comparative study for determination of root canal working length accuracy by different methods--an <i>in vivo/in vitro</i> study	They used fifty adult human single rooted teeth intended for extraction with mature apices
20.	Adriano LZ, et al. (2018) [33]	<i>In vitro</i> comparison between apex locators, direct and radiographic techniques for determining the root canal length in primary teeth	They compared the accuracy of EAL with the conventional radiographic techniques
21.	Rathore K, et al. (2020) [34]	Comparison of accuracy of apex locator with tactile and conventional radiographic method for working length determination in primary and permanent teeth	They compared the apex locator with a conventional radiographic method for working length determination in primary and permanent teeth.
22.	Davalbhakta RN, et al. (2021) [35]	Comparative evaluation of root ZX Mini® apex locator and digital radiography in determining the working length of primary molars: An <i>in vivo</i> study	They used tactile method as gold standard method for WL determination
23.	Goel T, et al. (2021) [36]	Comparative evaluation of working length using conventional radiographic method, radiovisiography, and apex locator in single-rooted permanent teeth	They have included permanent single rooted teeth
24.	Mousavi SA, et al. (2021) [37]	Comparative evaluation of root canal working length determination with three methods: conventional radiography, digital radiography and Raypex 6 apex locator: An experimental study	They have included permanent single rooted teeth
25.	Singh AK, et al. (2021) [38]	Evaluation of the efficacy of different systems in determination of root canal working length: A comparative study	They have included premolar teeth

Sr. no	Author and Year	Title	Reason for exclusion
26.	Ramezani M, et al. (2022) [39]	Accuracy of three types of apex locators versus digital periapical radiography for working length determination in maxillary premolars: An <i>in vitro</i> study	They have included premolar teeth
27.	Cardoso ML, et al. (2022) [40]	<i>In vitro</i> determination of working length in primary teeth	They have not mentioned about mean and SD values and not compared DR with apex locator
28.	Shibin J, et al. (2022) [41]	Evaluation of the working length determination accuracy by cone-beam computed tomography in primary teeth	They have evaluated CBCT, conventional radiography and apex locator. They haven't used DR

articles were assessed and checked for eligibility criteria. Following full-text screening, 28 articles (Table 4) were eliminated, as they were not in accordance to inclusion criteria [14-41]. Any inconsistency over final inclusion was discussed and resolved amongst two review authors (IA and SP), whereas, a third reviewer (FK) acted as mediator. Thus, ten full text articles that

meteligibility criteria and were included in present systematic review. Detailed summary of data selection was presented in the form of PRISMA 2020 flow diagram (Figure 1).

Study characteristics

The study characteristics of 10 included studies were listed in Table 5. The included studies were published

Table 5: Data extraction sheet; (ARCL: Actual root canal length, EAL: Electronic apex locator, WL: Working length, SD: Standard deviation, CBCT: Cone beam computed tomography, DR: Digital radiography)

Study ID	Author	Sample	Age group	Intervention	Comparison	Actual WL/ reference method	Outcome	Study design	Result	
									Mean ± SD	p value
1	Subramaniam P et al. (2005) [14]	22, single-rooted primary teeth	-	Formatron D 10 EAL	Digital radiographs with the digital sensor (Cygnus Media, Cygus Technologies, USA)	Actual root canal length (ARCL) of each tooth was measured under stereomicroscopy using direct observation of apical exit of k file	Higher similarity between apex locator measurements and actual canal length, followed by digital radiography and actual canal length, No significant difference was seen.	<i>In vitro</i>	EAL=15.94±2.06 DR=15.91±1.60 ARCL=15.53 ± 2.64	p> 0.05
2	Mello-Moura AC et al. (2010) [19]	20 primary incisors	-	Root ZX apex locator	RVG (Ultimate Image, Trophy, France)	ARCL of each tooth was measured at 15x stereomicroscopy magnification	EAL gave low absolute differences compared with digital radiographic method	<i>Ex vivo</i>	Absolute differences among the ARCL, RVG, EAL EAL=0.36 ± 0.30 RVG=1.40 ± 2.16	p< 0.05
3	Neena IE et al. (2011) [6]	30 primary teeth,90 canals	5-11 years	Apex locator	DR	Conventional radiographic method	No significant difference in the mean root length measurements in both technique	<i>In vivo</i>	Apex locator=11.79±1.70 DR=11.98 ±1.70 Conventional radiograph=11.76±1.67	p> 0.05
4	Tawil S et al. (2012)[15]	30 Extracted primary incisors	-	Root ZX, J. Morita Corporation, Tokyo, Japan	Digital x-ray sensor size # 1	ARCL was determined by advancing number 15K file until the tip of the file was showed by the naked eye to be with the level of the apical foramen	No significant difference between apex locator and digital X-Ray both showed lowest mean differences from actual length	<i>In vitro</i>	Apex locator=12.87±1.84 Digital X-Ray =12.89 ±1.82 ARCL =13.07 ±1.78	p> 0.05
5	Wankhade AD et al. (2013) [4]	70 extracted single rooted primary teeth	5-8 years	Joypex 5 (Denjoy Dental Co, Chin)	Size # 0 Schick CDR intraoral X-ray sensor (Schick Technologies, USA)	Stereomicroscopic examination under 8x magnification to determine ARCL	Group 1 (without PRR) EAL revealed statistically insignificant difference when com-	<i>In vitro</i>	EAL=16.43±0.79 DR=16.45±0.78 ARCL=16.44±0.79	EAL V/S ARCL >0.98 DR V/S ARCL <0.97

						pared with ARCL				
						Group 2 (with 1/4th PRR) EAL revealed statistically insignificant difference when compared with ARCL		EAL= 13.4±0.79 DR= 13.44±0.69 ARCL= 13.40±0.72	<0.96	<0.99
						Group 3 (with 1/4th to 3/4th PRR). DR showed a significant difference when compared with ARCL		EAL= 9.47±3.38 DR= 14.77±1.33 ARCL= 9.47±3.43	>0.99	<0.01
6	Kumar LV et al. (2016) [3]	22 children, 41 root canals (seven single-rooted and 15 multi-rooted canals)	6-15 years	Root ZX mini apex locator	RVG (Suni Medical Imaging Inc., California, USA)	Actual WL of each canal was measured (the apical exit of the file at the apical foramen or resorption bevel of the root is observed)	No significant difference between EAL and DR. Lowest mean difference was observed in the EWL group indicating that the use of EAL consistently brought the file tip closer to the apex	EAL=12.659±1.71 DR=13.037±1.50 Actual WL=12.67±1.70		p= 0.609
7	Sahni A et al. (2020) [16]	90 extracted single rooted primary teeth	-	DentaPort ZX (J Morita corp., Kyoto, Japan)	Digital radiograph sensor (Vatech EZ Sensor, Humanray Co. Ltd., Korea)	Actual WL was measured until the tip of the file was just visible at the apex/apical foramen or the apical resorption level.	No significant difference between EAL and DR. Electronic measurement was closer to actual WL as compared to digital radiography	EAL= 10.10 ± 1.78 DR = 10.08 ± 2.10 Actual WL= 10.36 ± 1.80		p= 0.066
8	Kayabasi M et al. (2020) [17]	20 extracted primary molars with resorption and 20 primary molars without resorption	-	COXO C Smart-1 Pro, iPex and Apex ID	RVG with a Size#1 sensor (CASTELLINI X-VS CMOS Radiography, Italy)	Actual WL was measured by inserting a size 15 K-file in the canal until the file tip became visible at the apical foramen under 6× magnification using a microscope	No statistically significant difference between the groups with and without root resorption. In the teeth with resorption the nearest measurements to actual WL were Apex ID > COXO C Smart-1 Pro > DR > iPex respectively. In the teeth without resorption the nearest measurements to actual WL were Apex ID > DR > COXO C Smart-1 Pro = iPex respectively	Teeth without root resorption Actual WL = 11.49±1.63 COXO = 10.92±1.52 iPex = 10.92±1.56 Apex ID = 11.18±1.57 DR = 11.03±1.64	Teeth with root resorption Actual WL = 9.53±1.44 COXO = 9.32±1.40 iPex = 9.22±1.38 Apex ID = 9.54±1.32 DR = 9.24±1.25	p= 0.931 p= 0.926
9	Pol DS et al. (2021) [18]	78 canals (30 extracted)	-	Propex II apex locator	DR (Schick Sirona, Germany)	Actual WL of each tooth was measured at 15X	EAL shows highest closer value to	Absolute difference of actual WL EAL = 0.007250±		p < 0.05

		primary molar)				magnification under stereomicroscope	actual WL thus provided better performance in working length determination in comparison to DR		0.2612 DR= 1.9570± 1.553		
10	Khan SA et al. (2022) [20]	84 root canals (58 primary teeth)	4–12 years	Root ZX mini Apex Locator (J Morita Corp, Tokyo, Japa)	DR	Actual WL of each canal was measured using Dental Loupes with 2.5X magnification	Statistically significant difference is seen in all the three groups	Ex vivo	Absolute differences among the actual WL, EAL and DR DR= 0.88± 0.79 EAL= -0.02 0.12	EAL V/S Actual WL 0.18	DR V/S Actual WL < 0.001

from January 1, 2005 to January 31, 2023. Five of the studies were *in vitro* study [42-46], four were *ex vivo* [3-4,47-48] and one was *in vivo* study [6]. No randomized and non-randomized clinical trials were found. The sample size of included studies ranged from 20-90 extracted human primary teeth. Age of the participants in the *in vivo* and *vivo* studies varied from five to fifteen years. EAL used in the intervention group were Formation D 10, Root ZX, Joypex 5, Root ZX mini, DentaPort ZX, COXO C Smart-1 Pro, iPex, Apex ID and Propex II, whereas DR used were size #0 and size #1. Accuracy was evaluated under stereomicroscopy using direct observation of apical exit of advancing K file, until tip of the file was visible at apical foramen or apical resorption level. Outcomes were assessed by comparing the difference among the actual length, DR and apex locator working length measurement. A statistically insignificant difference between EAL and DR was seen in seven out of 10 articles, whereas, other three studies showed statistically significant difference, indicating that EAL was more closely related to actual working length than

DR.

Risk of bias assessment

The methodological quality assessment of the selected studies using modified version of MINORS criteria was depicted in Figure 2. It demonstrates the reviewer’s assessment, regarding each risk of bias, which has been presented as percentages across all the included studies. This scale was modified because no clinical trials were found during the search study. Thus, only *in vivo*, *in vitro* and *ex vivo* studies were included. The scores were categorized as low, unclear, and high risk of bias. Low risk of bias indicates plausible bias that was not likely to change the results seriously, unclear risk of bias indicates bias that raised doubts about the results, and high risk of bias indicates bias that does not inspire confidence in the results.

The summary of risk of bias presented in Table 6 and Figure 2 show, seven studies by Mello Moura et al. [47], Wankhade et al. [4], Kumar et al. [3], Sahni et al. [44], Kayabasi et al. [45], Pol et al. [46] and Khan et al. [48], that presented low risk of bias which indicates

Table 6: Summary of risk of bias (MINORS: Methodological Index for Non-Randomized Studies, EAL: Electronic apex locator, DR: Digital Radiography)

S. no.	MINORS criteria	Scoring*									
		Study ID 1	Study ID 2	Study ID 3	Study ID 4	Study ID 5	Study ID 6	Study ID 7	Study ID 8	Study ID 9	Study ID 10
1	A clearly stated aim	2	2	2	2	2	2	2	2	2	2
2	Extracted Human primary teeth	0	2	1	1	2	2	2	2	2	2
3	Details of methodology-EAL and DR	1	2	1	2	1	2	2	2	2	1
4	Endpoints appropriate to the aim of the study	2	2	2	2	2	2	2	2	2	2
5	Unbiased assessment of the study endpoint	1	2	0	0	1	2	0	0	0	2
6	Prospective calculation of study size	0	0	0	0	0	0	0	0	0	0
7	An adequate control group	2	2	2	2	2	2	2	2	2	2
8	Baseline equivalence of groups	0	0	0	0	0	2	1	1	2	1
9	Adequate statistical analysis	2	2	2	2	2	2	2	2	2	2
Total score (out of 18)		10	14	10	11	12	16	13	13	14	14
Grading#		High risk	Low risk	High risk	High risk	Low risk	Low risk	Low risk	Low risk	Low risk	Low risk

*The items are scored 0 (not reported), 1 (reported but inadequate) or 2 (reported and adequate).
#GRADING: Low risk: score equal to 12 or greater than 12; High risk: score less than 12

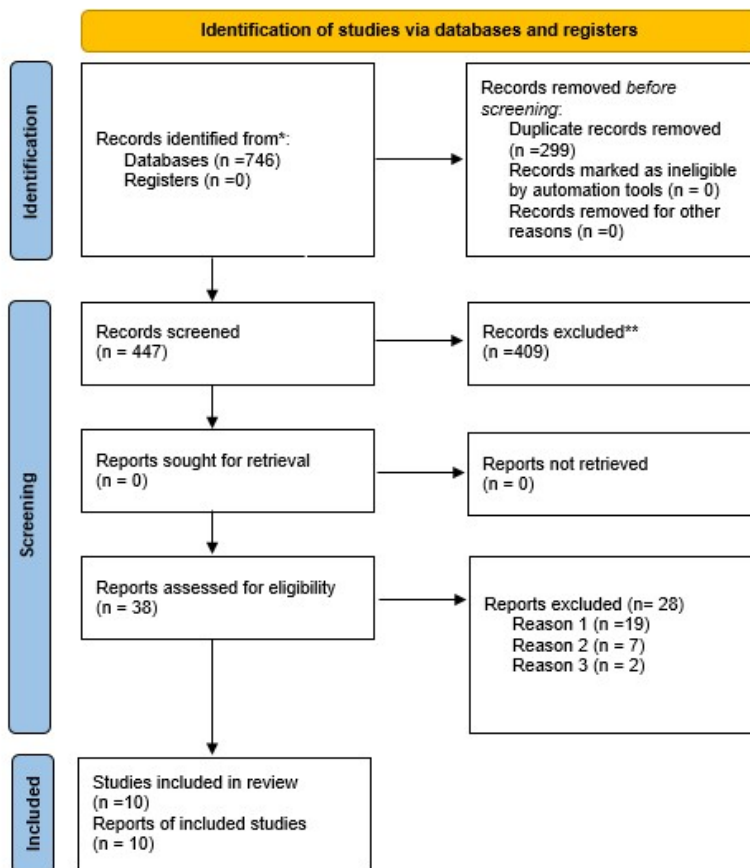


Figure 1: PRISMA 2020 flow diagram of the study

high quality of evidence.

The remaining three studies conducted by Subramaniam *et al.* [42], Neena IE *et al.* [6], and Sherif *et al.* [43], showed high risk of bias, which indicates low quality of evidence. The summarized findings show that the included studies are of moderate quality overall, with a high risk of bias evident only at definite points.

Discussion

Early loss of primary teeth can cause space closure resu-

lting in malocclusion of permanent dentition. Pulpectomy procedure involves complete removal of both coronal and radicular pulp. WL determination is an essential step in pulpectomy procedure, as it decides the position of apical foramen and thus the extent of obturation.

It is hard to judge the root canal anatomy of primary teeth because of continuous ongoing resorption and root canal shape. [49] The position of canal terminus and measurement of WL can be done by various techniques.

One of the widely used methods is the radiographic

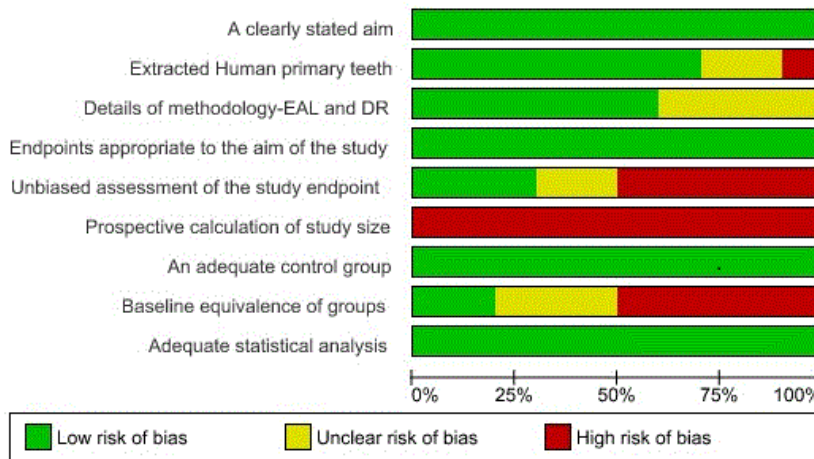


Figure 2: Risk of bias graph: review author’s judgments about each risk of bias item presented as percentages across all included studies

method for WL determination. However, measurement by this method is generally one or a half-millimeter (mm) short of the radiographic apex, where the apical constriction is generally thought to be located [50]. To eliminate the many problems associated with the radiographic methods, apex locator is now being used clinically and has become an essential part of the armamentarium of root canal procedure. Several studies have compared WL determination done by EAL and DR in primary teeth; only nine studies have been considered for inclusion in this systematic review.

The sample size is important to make any inferences about a population from a sample. Sample size was 20 to 90 primary teeth for the included studies. None of the studies revealed any details about the sample size calculation. This could lead to an increased chance of risk of bias of individual studies. The amount of physiologic root resorption can affect the determination of WL in an endodontic procedure. Amount of root resorption was reported in majority of the studies, however, three studies, Subramaniam P *et al.* [42], Neena IE *et al.* [6] and Sherif B *et al.* [43], inadequately reported the amount of root resorption. The threshold file size for working length measurements should be size # 15 K, as the tip diameter of the No # 10K files is less than 120 micrometers, which is not identifiable [6]. This finding was in accordance with studies by Kumar L V *et al.* [3], Sherif B *et al.* [43] and Sahni A *et al.* [44], Kayabasi M *et al.* [45]. Density profile plot analysis for digital images found that size #20 files were employed for radiographic length computation, because size #15 and size #10 files have decreasing perceptibility of file length [51].

Because of anatomical variances, anatomical structure interference, and projection problems, determining the precise radiographic root canal length is difficult [52]. Kumar LV *et al.* [3], Mello Moura *et al.* [47], Neena IE *et al.* [6], Sherif B *et al.* [43] and Kayabasi M *et al.* [45] employed the paralleling technique which is difficult to perform on paediatric patients. However, in the remaining four studies, they have not reported about the projection technique. These variables may result in over-instrumentation and over-filling of canals, causing permanent tooth bud injury [1,53].

As calibrated digital measurements are more accurate than un-calibrated ones [54], digital image calibration was performed, prior to WL determination, using

an on-screen calibration tool. Kim *et al.* [55] demonstrated in their study that radiographic measurement of WL using an onscreen straight-line measurement was effective.

Apex locators are classified based on their generations. The first and second generations of EALs are obsolete, and are no longer manufactured or utilized in the modern era of dentistry. Nasiri *et al.* [56] performed a systematic review and meta-analysis and found that all generations are equally beneficial and accurate in WL evaluation.

The real WL was calculated by subtracting 0.5mm from the distance between the apical foramen and the apical constriction, which is roughly 0.5-1.0 mm [57]. A 0.5 mm margin was employed in numerous researches evaluating the accuracy of WL. Amongst the included studies, five studies, by Kumar LV *et al.* [3], Sahni *et al.* [44], Kayabasi M *et al.* [45], Pol DS *et al.* [46] and Khan SA *et al.* [48], determined WL by subtracting 0.5mm from apical foramen, while five studies by Wankhade AD *et al.* [4], Neena IE *et al.* [6], Subramaniam P *et al.* [42], Sherif B *et al.* [43] and Mello Moura *et al.* [47] did not report about the same. When compared to DR, it was found that the WL measurement provided by the EAL was near to the real WL determination in all of the included studies. This was in line with a number of research studies [42,58] that measured the precision of the apex locator in primary teeth. The radiographic length determination is difficult in primary teeth because of constant change in apex position due to continuous ongoing root resorption. However, only a few studies have found that in roots with wider apical foramen, EAL measurements are much shorter than the true WL [59]. In primary dentition, however, most studies found EAL accuracy rates of 64 to 96 percent [58, 60]. In a study by Sahni *et al.* [44], a substantial correlation was discovered between the WL of the reference technique and EAL, and this was in agreement with Shabahang *et al.* [61], who concluded that EAL reliably determines the root end even in cases when root resorption is present. Furthermore, this is consistent with the findings of other researchers who reported the great accuracy of EALs in primary teeth.

The disparity in accuracy of WL may be due to variation in study designs, sample sizes, rate of resorption, file size, reference point, radiographic technique, and di-

fferent generations of EAL used in the included studies.

This review has some limitations, one of which was usage of limited databases for search strategy. Another limitation was use of English literature only as, articles published in other languages were excluded. Finally, caution should be exercised before applying the results of this review in a clinical scenario, as all the included studies were of *in vitro* design.

Conclusion

Within the limitation of present systematic review, we found moderate quality of evidence to suggest accuracy of EAL and DR for WL determination. Majority of studies showed statistically insignificant difference between EAL and DR. However, in few studies, electronic measurement was close to actual WL as compared to DR. Based on the evidence that is currently available, EAL can be considered as an alternative for working length measurement in primary teeth. However, future research should include information about the study populations, blinding and sufficient documentation.

Conflict of Interest

The authors declare that they have no conflict of interest.

References

- [1] Leonardo MR, Silva LA, Nelson-Filho P, Silva RA, Rafini MS. *Ex vivo* evaluation of the accuracy of two electronic apex locators during root canal length determination in primary teeth. *Int Endod J*. 2008; 41: 317–321.
- [2] American Association of Endodontists. Glossary of endodontic terms. American Association of Endodontists; 2003. Available at: <https://www.worldcat.org/title/glossary-of-endodontic-terms/oclc/54406300>
- [3] Kumar LV, Sreelakshmi N, Reddy ER, Manjula M, Rani ST, Rajesh A. Clinical evaluation of conventional radiography, radiovisio-graphy, and an electronic apex locator in determining the working length in primary teeth. *Pediatr Dent*. 2016; 38: 37-41.
- [4] Wankhade AD, Kumar R, Singh RK, Chandra A. Root canal length determination by different methods in primary teeth: an *in vivo* study. *Pediatr Dent*. 2013; 35: 38-42.
- [5] Odabaş ME, Bodur H, Tulunoğlu O, Alaçam A. Accuracy of an electronic apex locator: A clinical evaluation in primary molars with and without resorption. *J Clin Pediatr Dent*. 2011; 35: 255-258.
- [6] Neena IE, Ananthraj A, Praveen P, Karthik V, Rani P. Comparison of digital radiography and apex locator with the conventional method in root length determination of primary teeth. *J Indian Soc Pedod Prev Dent*. 2011; 29: 300-304.
- [7] Shearer AC, Horner K, Wilson NH. Digital radiography for imaging root canals: an *in vitro* comparison with conventional radiography. *Quint Int*. 1990; 21: 789-794.
- [8] Ghaemmaghamis S, Eberie J, Duperon D. Evaluation of Root ZX apex locator in primary teeth. *Pediatr Dent*. 2008; 30: 496–498.
- [9] Beltrame AP, Triches TC, Sartori N, Bolan M. Electronic determination of root canal working length in primary molar teeth: an *in vivo* and *ex vivo* study. *Int Endod J*. 2011; 44: 402-406.
- [10] Page MJ, Moher D, Bossuyt PM, Boutron I, Hoffmann TC, Mulrow CD, et al. PRISMA 2020 explanation and elaboration: updated guidance and exemplars for reporting systematic reviews. *BMJ*. 2021; 372.
- [11] Chokkalingam A, Scherer R, Dickersin K. Agreement of data in abstracts compared to full publications. *Control Clin Trials* 1998; 19: S61–S62.
- [12] Slim K, Nini E, Forestier D, Kwiatkowski F, Panis Y, Chipponi J. Methodological index for non-randomized studies (minors): development and validation of a new instrument. *ANZ J Surg*. 2003; 73: 712-716.
- [13] Cohen J. A coefficient of agreement for nominal scales. *Educ Psychol Meas*. 1960; 20: 37-46.
- [14] Shanmugaraj M, Nivedha R, Mathan R, Balagopal S. Evaluation of working length determination methods: an *in vivo/ ex vivo* study. *Indian J Dent Res*. 2007; 18: 60-62.
- [15] Krajczár K, Marada G, Gyulai G, Tóth V. Comparison of radiographic and electronic working length determination on palatal and mesio-buccal root canals of extracted upper molars. *Oral Surg Oral Med Oral Pathol Oral Radiol Endod*. 2008; 106: e90-e93.
- [16] Krajczár K, Soltész MZ, Gyulai G, Marada G, Szabó G, Tóth V. ProPex apexlokátorral és radiológiai módszerrel végzett munkahossz-meghatározás összehasonlítása *in vitro* direkt eljárással [Direct comparison of working length determination by ProPex electronic apex locator and radiographic method--an *in vitro* study]. *Fogorv Sz*. 2008; 101: 107-111.
- [17] Ravanshad S, Adl A, Anvar J. Effect of working length measurement by electronic apex locator or radiography

- on the adequacy of final working length: a randomized clinical trial. *J Endod.* 2010; 36: 1753-1756.
- [18] Cianconi L, Angotti V, Felici R, Conte G, Mancini M. Accuracy of three electronic apex locators compared with digital radiography: an *ex vivo* study. *J Endod.* 2010; 36: 2003-2007.
- [19] Real DG, Davidowicz H, Moura-Netto C, Zenkner Cde L, Pagliarin CM, Barletta FB, de Moura AA. Accuracy of working length determination using 3 electronic apex locators and direct digital radiography. *Oral Surg Oral Med Oral Pathol Oral Radiol Endod.* 2011; 111: e44-e49.
- [20] Parekh V, Taluja C. Comparative study of periapical radiographic techniques with apex locator for endodontic working length estimation: an *ex vivo* study. *J Contemp Dent Pract.* 2011; 12: 131-134.
- [21] Vieyra JP, Acosta J, Mondaca JM. Comparison of working length determination with radiographs and two electronic apex locators. *Int Endod J.* 2010; 43: 16-20.
- [22] Vieyra JP, Acosta J. Comparison of working length determination with radiographs and four electronic apex locators. *Int Endod J.* 2011; 44: 510-518.
- [23] Saritha S, Uloopi KS, Vinay C, Chandra Sekhar R, Rao VV. Clinical evaluation of Root ZX II electronic apex locator in primary teeth. *Eur Arch Paediatr Dent.* 2012; 13: 32-35.
- [24] Singh SV, Nikhil V, Singh AV, Yadav S. An *in vivo* comparative evaluation to determine the accuracy of working length between radiographic and electronic apex locators. *Indian J Dent Res.* 2012; 23: 359-362.
- [25] Kishor KM. Comparison of working length determination using apex locator, conventional radiography and radiovisiography: an *in vitro* study. *J Contemp Dent Pract.* 2012; 13: 550-553.
- [26] Mandlik J, Shah N, Pawar K, Gupta P, Singh S, Shaik SA. An *in vivo* evaluation of different methods of working length determination. *J Contemp Dent Pract.* 2013; 14: 644-648.
- [27] Oznurhan F, Ünal M, Kapdan A, Ozturk C, Aksoy S. Clinical evaluation of apex locator and radiography in primary teeth. *Int J Paediatr Dent.* 2015; 25: 199-203.
- [28] Basso MD, Jeremias F, Cordeiro RC, Santos-Pinto L. Digital radiography for determination of primary tooth length: *in vivo* and *ex vivo* studies. *Sci World J.* 2015; 2015: 939045.
- [29] Singh D, Tyagi SP, Gupta S, Jain A. Comparative evaluation of adequacy of final working length after using Raypex5 or radiography: an *in vivo* study. *J Indian Soc Pedod Prev Dent.* 2015; 33: 208-212.
- [30] Carneiro JA, de Carvalho FM, Marques AA, Junior EC, Garcia LD, Goncalves LC. Comparison of working length determination using apex locator and manual method - *ex vivo* study. *Dent Med Res.* 2016; 4: 39-43.
- [31] Dutta K, Desai PD, Das UK, Sarkar S. Comparative evaluation of three methods to measure working length - Manual tactile sensation, digital radiograph, and multidetector computed tomography: An *in vitro* study. *J Conserv Dent.* 2017; 20: 76-80.
- [32] Khateeb SU, Kaul K, Kaul R, Jeri SY, Ahmad R. Comparative study for determination of root canal working length accuracy by different methods: an *in vivo/in vitro* study. *IP Annals Prosth Rest Dent.* 2017; 3: 88-93
- [33] Adriano LZ, Barasuol JC, Cardoso M, Bolan M. In vitro comparison between apex locators, direct and radiographic techniques for determining the root canal length in primary teeth. *Eur Arch Paediatr Dent.* 2019; 20: 403-408.
- [34] Rathore K, Tandon S, Sharma M, Kalia G, Shekhawat T, Chundawat Y. Comparison of Accuracy of Apex Locator with Tactile and Conventional Radiographic Method for Working Length Determination in Primary and Permanent Teeth. *Int J Clin Pediatr Dent.* 2020; 13: 235-239.
- [35] Davalbhakta RN, Gokhale NS, Hugar SM, Badakar CM, Gowtham A, Soneta SP. Comparative evaluation of root ZX Mini® apex locator and radiovisiography in determining the working length of primary molars: An *in vivo* study. *J Oral Biol Craniofac Res.* 2021; 11: 257-262.
- [36] Goel T, Indushekar KR, Saraf BG, Sheoran N, Sardana D, Chawla M. Comparative evaluation of working length using conventional radiographic method, radiovisiography, and apex locator in single-rooted permanent teeth. *J Oral Health Comm Dent.* 2021; 15: 49-54.
- [37] Mousavi SA, Zahedinejad A, Kowsari B, Kolahdouzan E, Mousavi SI, Saeidian S. Comparative evaluation of root canal working length determination with three methods: conventional radiography, digital radiography and raypex6 apex locator: an experimental study. *J Dent Mater Techniq.* 2021; 10: 87-93.
- [38] Singh AK, Rathod A, Reddy A, Moyin S, Punathil S, Shah A. Evaluation of the efficacy of different systems in determination of root canal working length: A comparative study. *World J Dent.* 2021; 12: 399-402.
- [39] Ramezani M, Bolbolian M, Aliakbari M, Alizadeh A, Tofangchiha M, Faegh SM, et al. Accuracy of three types

- of apex locators versus digital periapical radiography for working length determination in maxillary premolars: An *in vitro* study. Clin Pract. 2022; 12: 1043-1053.
- [40] Cardoso ML, Lugo de Langhe CD, Diaz NG. *In vitro* determination of working length in primary teeth. Univ Odontol. 2022; 41.
- [41] Shibin J, Gs P, M S, S N, Adimoulame S, M K. Evaluation of the working length determination accuracy by cone-beam computed tomography in primary teeth. Int J Clin Pediatr Dent. 2022; 15(Suppl 1): S92-S96.
- [42] Subramaniam P, Konde S, Mandanna DK. An *in vitro* comparison of root canal measurement in primary teeth. J Indian Soc Pedod Prev Dent. 2005; 23: 124-125.
- [43] Sherif B, El Tawil. An *in vitro* comparison of root canal Length measurements of primary teeth using different techniques. J Am Sci. 2012; 8: 541-547.
- [44] Sahni A, Kapoor R, Gandhi K, Kumar D, Datta G, Malhotra R. A comparative evaluation of efficacy of electronic apex locator, digital radiography, and conventional radiographic method for root canal working length determination in primary teeth: An *in vitro* study. Int J Clin Pediatr Dent. 2020; 13: 523-528.
- [45] Kayabasi M, Oznurhan F. Evaluation of the accuracy of electronic apex locators, cone-beam computed tomography, and digital radiography in primary teeth: An *in vitro* study. Microsc Res Tech. 2020; 83: 1330-1335.
- [46] Pol SD, Katge FA, Poojari MS, Shetty SK, Patil DP. Accuracy of working length determination using three different methods: An *in vitro* study. Nair hospital dental college J Contemp Dent. 2021; 1: 3-8.
- [47] Mello-Moura AC, Moura Netto C, Araki AT, Guedes-Pinto AC, Mendes FM. *Ex vivo* performance of five methods for root canal length determination in primary anterior teeth. Int Endod J. 2010; 43: 142-147.
- [48] Khan SA, Khanna R, Navit S, Jabeen S, Grover N, Pramanik S. Comparison of Radiovisiography, an Apex Locator and an Integrated Endomotor-inbuilt Apex Locator in Primary Teeth Endometrics. Int J Clin Pediatr Dent. 2022; 15(Suppl 1): S18-S21.
- [49] American Academy of Paediatric Dentistry. Guideline on pulp therapy for primary and immature permanent teeth. Reference manual 2009-2010. Pediatr Dent. 2009; 33: 212-219.
- [50] Hassanien E, Hashem A, Chalfin H. Histomorphometric study of the root apex of mandibular premolar teeth: an attempt to correlate working length measured with electronic and radiographic methods to various positions in the apical portion of the canal. J Endod. 2008; 34: 408-412.
- [51] Hör D, Krusy S, Attin T. *Ex vivo* comparison of two electronic apex locators with different scales and frequencies. Int Endod J. 2005; 38: 855-859.
- [52] Haffner C, Folwaczny M, Galler K, Hickel R. Accuracy of electronic apex locators in comparison to actual length an *in vivo* study. J Dent. 2005; 33: 619-25.
- [53] Holan G, Fuks AB. A comparison of pulpectomies using ZOE and KRI paste in primary molars: a retrospective study. Pediatr Dent. 1993; 15: 403-407.
- [54] Loushine RJ, Weller N, Kimbrough WF, Potter BJ. Measurement of endodontic file lengths: calibrated versus uncalibrated digital images. J Endod. 2001; 27: 779-781.
- [55] Kim-Park MA, Baughan IW, Hartwell GR. Working length determination in palatal roots of maxillary molars. J Endod. 2003; 29: 58-61.
- [56] Nasiri K, Wrbas KT. Accuracy of different generations of apex locators in determining working length; a systematic review and meta-analysis. Saudi Dent J. 2022; 34: 11-20.
- [57] Dummer PM, McGinn JH, Rees DG. The position and tomography of the apical canal constriction and apical foramen. Int Endod J. 1984; 17: 192-198.
- [58] Kielbassa AM, Muller U, Munz I, et al. Clinical evaluation of the measuring accuracy of ROOT ZX in primary teeth. Oral Surg Oral Med Oral Pathol Oral Radiol Endod 2003; 95: 94-100.
- [59] Berman LH, Fleischman SB. Evaluation of the accuracy of the Neosono-D electronic apex locator. J Endod 1984; 10: 164-167.
- [60] Goerig AC, Camp JH. Root canal treatment in primary teeth: a review. Pediatr Dent. 1983; 5: 33-37.
- [61] Shabahang S, Goon WWY, Gluskin AH. An *in vivo* evaluation of root ZX electronic apex locator. J Endod. 1996; 22: 616-618.